

Manual

EQF 3300

Rn/Th gas and Rn/Th progeny monitor

Version 07/2025

Reference documents:

Software manual dVISION

SARAD GmbH

Wiesbadener Straße 10

01159 Dresden

www.sarad.de

info@sarad.de



Content

Operational controls.....	5
Basic equipment	5
Sampling head for progeny products	6
1. Overview.....	7
1. 1. The DACM32 platform as basic equipment.....	7
1. 2. Control of the measurement process- measuring cycles	7
1. 3. Alarm-system.....	7
1. 4. Event -memory	8
1.5. Communication with the host-system	8
2. Operation	9
2. 1. Switching ON/OFF , standby-mode, Fuse.....	9
2. 2. Power supply	9
2. 3. Operation panel (Touchscreen).....	9
2. 4. Interfaces.....	10
2. 4. 1. Interfaces for communication (COM1, COM2).....	10
2. 4. 2. Analog output	10
2. 4. 3. Sockets for external accessories (AUX1, AUX2).....	11
2. 5. Data storage of measurements	11
2. 6. Menu navigation.....	12
2. 6. 1. Main page	12
2. 6. 2. Display of module information and module settings	13
2. 6. 3. Display of component configuration	14
2. 6. 4. Selection of measurement cycle	15
2. 6. 5. Display of actual measured values	15
2. 6. 6. Display of the stored measurement values	15
2. 6. 7. Graphical display of the measurement data as a time series	16
2. 6. 8. Display of basic data	18
2. 6. 9. Alarm-display	19
2. 6. 10. Display of event memory.....	20
2. 7. Setup (timer, synchronous start, display switch off).....	20
2. 7. 1. Timer.....	20
2. 7. 2. Synchronous start at a set time of day.....	21
2. 7. 3. Display shutdown interval	21
2. 8. The integrated GPS receiver	21

3. Sensors and actuators in the EQF 3300.....	22
3. 1. Radon measurement, temperature and relative humidity	22
3. 1. 1. Measuring principle	22
3. 1. 2. DACM32-components for the radon measurement	23
3. 1. 3. Display of measuring values for radon, temperature and humidity	23
3. 2. Radon progeny product measurement	23
3. 2. 1. Functional principle	23
3. 2. 2. DACM32-components for radon progeny products	24
3. 2. 3. Display of radon progeny products	24
3. 3. Flow measurement, flow control and pump current	24
3. 3. 1. Functional principle	24
3. 3. 2. DACM32-components for internal air circuit	24
3. 3. 3. Display of the measured values of the air circuit	24
3. 4. Barometric pressure, differential pressure (option)	25
3. 5. Warning and alarm lights	25
3. 6. The connectors „AUX1“ and „AUX2“	25
4. EQF 3300 device configuration.....	26
4. 1. Predefined measuring cycles.....	26
4. 2. Predefined warnings and alarms.....	27
5. Important hints on operating the device	28
5. 1. Vibrations and strong electromagnetic fields	28
5. 2. Aggressive Gases	28
5. 3. Environmental conditions	28
5. 4. Control of the alpha spectra.....	28
5. 5. Avoiding condensation	28
5. 6. Water ingress protection.....	29
5. 7. Filter at the air inlet of the device	29
5. 8. Rechargeable battery	29
5. 9. Hints for the sampling head for progeny products	30
5. 9. 1. Connection and placing	30
5. 9. 2. Change of the filter	30
5. 9. 3. Detector cleaning and protection.....	30
6. Use of accessories	31
6. 1. Accessory adapter	31
6. 2. Measuring case for harsh environmental conditions.....	31
6. 3. Light column	31

Attachment.....	33
A) DACM32 components	33
A1 – Type of components of DACM32	33
A2 – Overview of the used components in EQF 3300.....	33
B) Connector pin assignment	34
C) Disposal instructions	35

Operational controls

Basic equipment

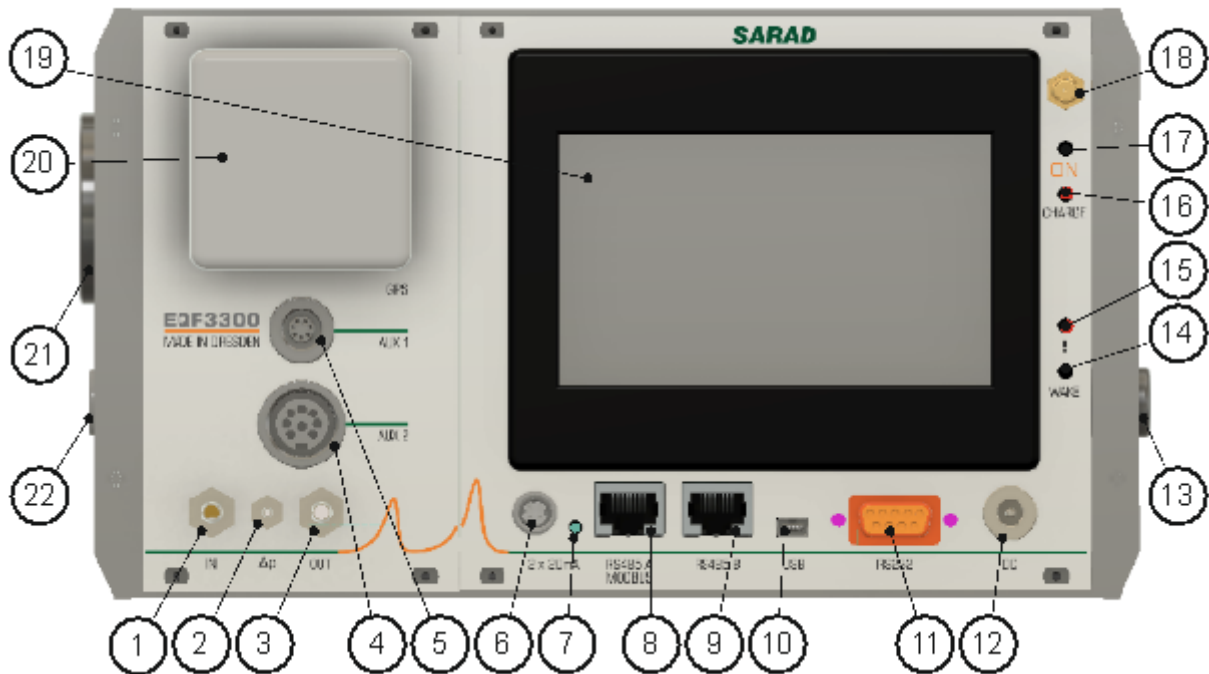


fig 1: basic equipment

- 1) Internal air circuit air inlet
- 2) Connection for differential pressure measurement
- 3) Internal air circuit air outlet
- 4) Accessory socket "AUX2" for connecting signal lights
- 5) Accessory socket "AUX1" for connecting the radon progeny measurement head
- 6) Connection socket for 2x 0-20 mA current loop outputs
- 7) LED indicator for activated current loop outputs
- 8) RS485A interface (configurable for MODBUS RTU protocol)
- 9) RS485B interface
- 10) USB Type B Mini interface
- 11) RS232 interface
- 12) Connection socket for power supply
- 13) Device fuse
- 14) Button for activating the display
- 15) LED indicator for alarms/warnings
- 16) LED indicator for charging status
- 17) Power ON button
- 18) WIFI socket
- 19) Coloured touchscreen display
- 20) GPS receiver
- 21) Accessory adapter (RP-head, water intake protection (optional))
- 22) Connection socket for water ingress protection (optional)

Sampling head for Radon/Thoron progeny

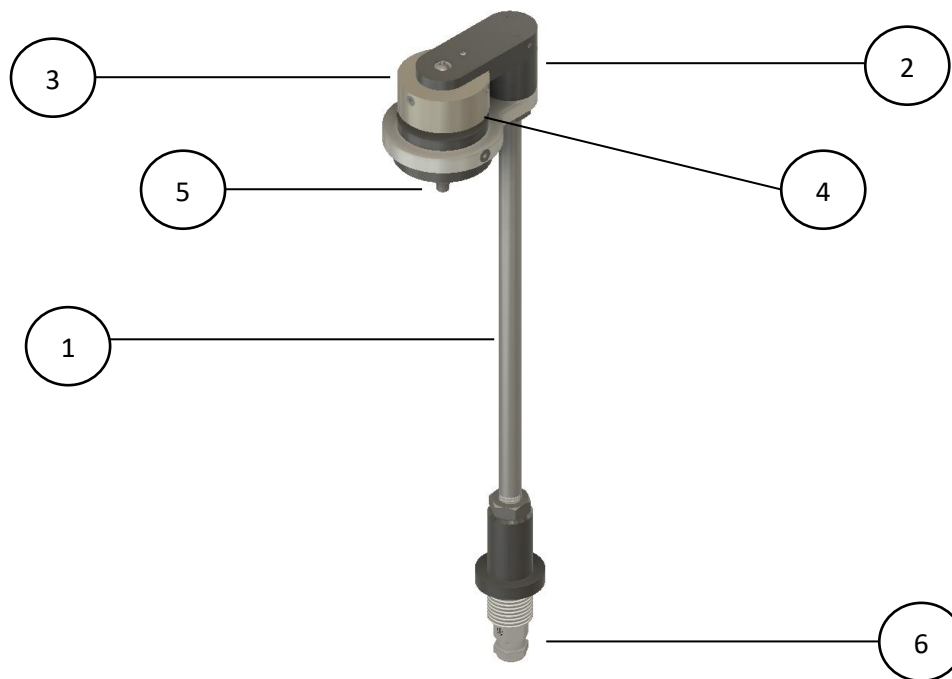


fig 2: Sampling head for progeny products

- 1) Rod
- 2) Swivel arm
- 3) Detector
- 4) Filter cap
- 5) Tube connector for connecting air tube between the RP-head and air inlet of the basic unit
- 6) Connection socket for connecting cable between the RP/head and the "AUX1" socket of the basic unit

1. Overview

1.1. The DACM32 platform as basic equipment

The device is based on the DACM32 measurement platform developed by SARAD. This platform is based on a microcontroller with proprietary firmware. Since no operating system is used and communication also takes place via proprietary protocols, maximum protection against tampering is guaranteed.

The DACM32 platform is based on hardware with a number of universal interfaces to which a wide variety of sensors and actuators can be connected. Simple examples are an analog input and a switching output. These interfaces are referred to as components in the DACM32, and the different types of interfaces are referred to as component types. Each component can be parameterized using configuration software to calculate the respective measured values in the desired physical unit from the sensor's electrical output signal. Each component is uniquely indexed in the DACM32 and has a unique name. This consists of an abbreviation for the component type followed by an index if multiple components of a type are present (example: AIN2 refers to analog input no. 2). Each component is assigned an alias name via configuration that identifies the component in a user-friendly manner. Depending on requirements, the short names or alias names are used on the device display, in the configuration software, and in the operating software. The appendix contains a list of all component types with a brief functional description.

A specific measuring device is created by combining the DACM32 hardware with the required sensors and actuators, as well as the associated component and device configuration. Standard users do not need to worry about these aspects, as the devices are fully configured for the respective measurement task upon delivery. However, familiarity with the platform concept will help you better understand this manual. Furthermore, both device manufacturers and experienced users can implement customized modifications quickly and easily.

1.2. Control of the measurement process- measuring cycles

A measurement cycle defines the time interval at the end of which the measured values acquired during this interval are stored in the data memory. Depending on the definition, the measurement cycle is repeated for a defined number of measurements or indefinitely, so that the measurement data is available as a time series. Up to 15 measurement cycles can be stored in the device, customized for the respective measurement task. The required measurement cycles for all standard applications are already included upon delivery. The measurement cycles are defined using configuration software, allowing experienced users to create their own cycles.

Within a measurement cycle, each component can be controlled individually. It is defined which components are included in a measurement – and when within a cycle a component should generate data or activate actuators.

1.3. Alarm-system

A maximum of 32 independent alarms can be freely defined. Any measurement value available in the device can be used as the data source for an alarm. A distinction is made between alarms for current sample values (measurement and verification every second) and interval alarms (verification of the

integral values at the end of the interval). An alarm is acknowledged either via the touch panel, a communication interface, or (if provided in the device) via an input for connecting a button. The types of acknowledgement permitted can be determined via configuration. An on and off threshold can be defined for each alarm, allowing the implementation of a hysteresis. If the on threshold is greater than the off threshold, an alarm is generated when the measured value increases; otherwise, an alarm is generated when the measured value decreases. Each alarm can be assigned several actions that are executed by the corresponding components (e.g., activating a signal light via a switching output). The alarm settings configured in the device are described in the "Predefined Warnings and Alarms" section.

1.4. Event -memory

The last 100 important events affecting the device are stored in the event log with a time stamp. This log cannot be deleted by the user, so errors, alarm situations, and tampering with the device can be traced later. The following events are recorded:

- Turning the device on and off
- Setting the device clock
- Changes to the component or device configuration
- Selecting a measurement cycle
- Starting and stopping the measurement
- Occurred alarms
- Acknowledgment of alarms

1.5. Communication with the host-system

All device settings, data transfer, and remote control of the device are performed independently of the communication channel using a proprietary protocol. This protocol is used by all SARAD software solutions. Additionally, current measurement data can be retrieved via the industry-standard "MODBUS RTU" protocol. Separate applications are available for device configuration (dCONFIG) and device operation (dVISION).

2. Operation

2. 1. Switching ON/OFF, standby-mode, fuse

For safety reasons, the device is shipped with the removed fuse. Before switching the device on, please open the fuse holder on the right side of the housing, insert the fuse, and then close the fuse holder again. Press the "ON" power button and hold it for a few seconds until the SARAD logo appears on the display. The device is switched off using the "OFF" touch button in the main menu (top centred).

After completing a measurement, the device goes into "standby" mode so that the device is not completely disconnected from the internal battery. The display is deactivated after a configurable time interval. The display is activated by pressing the "WAKE" button.

If the device is not used for an extended period of time, the battery should be fully charged and disconnected from the power supply by switching it off using the "OFF" touch button in the main menu on the display. The fuse must be removed for shipping or air transport.

2. 2. Power supply

The device contains a NiMH battery with a nominal voltage of 12V and a capacity of 7.6Ah. Power consumption during measurement depends on the device configuration and the components/sensors used in the measurement cycle. To maximize battery operating time, use only the components/sensors actually required.

The battery is charged using the included plug-in power adapter (18-20V/60VA). The integrated charging circuit allows the battery to be fully charged within four hours. The "DC" connection socket for the power adapter is located at the bottom right of the front panel of the device. The red LED indicator to the right of the display lights up during charging. It goes out when the battery is fully charged.

The device can be operated continuously with the power supply. The charging control ensures cyclic charging to optimize battery life. During the charging process, heat is released, which causes the entire device to heat up. The integrated temperature sensor then displays significantly elevated values. To accurately measure the outside temperature, an additional sensor separate from the device should be used in the case of continuous mains operation.

If the battery voltage drops below 11.2V during a measurement, the measurement is aborted. If the discharge continues below a threshold of 10.6V, the deep discharge protection completely shuts down the device's electronics. The device can only be switched on again once the battery voltage has reached the threshold of 11.6V during the charging process.

The battery should always be charged at temperatures between 10°C and 30°C. At ambient temperatures above 40°C, charging is automatically interrupted to protect the battery. When not in use, the device should be turned off using the "OFF" touch button in the main menu.

2. 3. Operation panel (Touchscreen)

The device is operated via touchscreen. The display and backlight consume a relatively high amount of power, so they automatically shut off even during a measurement if no input is made. The time from the last touch to shutdown can be set to a maximum of 255 seconds via the device setup.

The display is activated as soon as the black "WAKE" push button is pressed. The last displayed page is always activated afterward. All other operating functions are controlled via the dynamic touch buttons shown on the display.

2. 4. Interfaces

2. 4. 1. Interfaces for communication (COM1, COM2)

The device has two independent communication channels (COM1, COM2) that can be used to communicate with the device simultaneously. Different physical interfaces are assigned to each channel, which are automatically switched between according to a priority scheme.

The following interfaces are assigned to the COM1 communication channel:

- USB: active as soon as a USB connection is established
- RS232: active when an RS232 signal is detected and no USB connection is present
- RS485B: active when neither a USB nor an RS232 connection is present

The COM1 communication channel cannot be configured using configuration software. This ensures constant access to the device. The data transfer speed can be increased by pressing the "COM1" button in the main menu.

The following interfaces are assigned to the COM2 communication channel:

- WLAN: active when WLAN has been activated by the user and the device is logged in
- RS485A: active when the device is not logged in to the WLAN

The COM2 communication channel is configured using the setup functions of the configuration software. The following modes are available:

- SARAD 9600 bps no parity
- SARAD 115200 bps no parity
- MODBUS 9600 bps even parity
- MODBUS 19200 bps even parity
- SARAD wireless

The modes marked with "SARAD" use the proprietary SARAD protocol. This includes data transfer and complete device control.

The industry standard MODBUS RTU is also supported. This protocol only supports querying current measured values. Information on using the MODBUS RTU protocol can be found in the document "AN-009-sarad_modbus_rtu_protocol".

The "SARAD wireless" setting must be selected to activate the WLAN interface. If WLAN is not used, this mode should not be selected, as operating the wireless interface consumes a relatively high amount of power. Once this mode is enabled, the device will only switch to the WLAN connection once it is logged in. The WLAN access data (SSID, password, server, and port) must be entered in the setup function of the configuration software.

2. 4. 2. Analog output

The device has two freely configurable current loop outputs, which are available at the "2 x 20mA" socket. The following output signal options are available:

- 0...20mA
- 4...20mA
- 0...24mA

Each output can be assigned any measured value acquired in the device. The desired value range of the measured value must be assigned to the selected output range (e.g., for battery voltage: 4...20mA corresponds to 0...15V). All settings are made using the setup function within the configuration software.

2. 4. 3. Sockets for external accessories (AUX1, AUX2)

The two sockets provide additional components of the DACM32. They can be used to control external accessories or integrate external sensors into the system. In addition to the standard configuration, device- and user-specific modifications are possible. The standard configuration is documented in the section "AUX1 and AUX2 Connectors." Customer-specific configurations are described in a separate document.

2. 5. Data storage of measurements

The measurement data is stored on an internal SD card. Several million data records can be stored. The generated measurement data is always saved as raw data, i.e., in the binary format generated by the components. This ensures absolute traceability of the measurement data for quality assurance purposes. A component can generate one or more measured variables from the raw data. To display the measured values on the device or to retrieve current measured values via the communication interface, they are calculated based on the raw data using the component configuration. When transferring the complete measurement data to the host system, however, only the compressed raw data is transferred along with the component configurations. The host system then generates the actual measurement results from this.

Please note that the device can collect very large amounts of measurement data, which later result in longer transmission times via the communication interfaces. Therefore, only activate the required sensors and select the length of the measurement intervals appropriate to your application.

The data of the memory card can be deleted using the corresponding function in the operating software.

2. 6. Menu navigation

2. 6. 1. Main page

After activating the display using the button below the display, the main navigation page appears.



fig 3: Main menu if measurement stopped

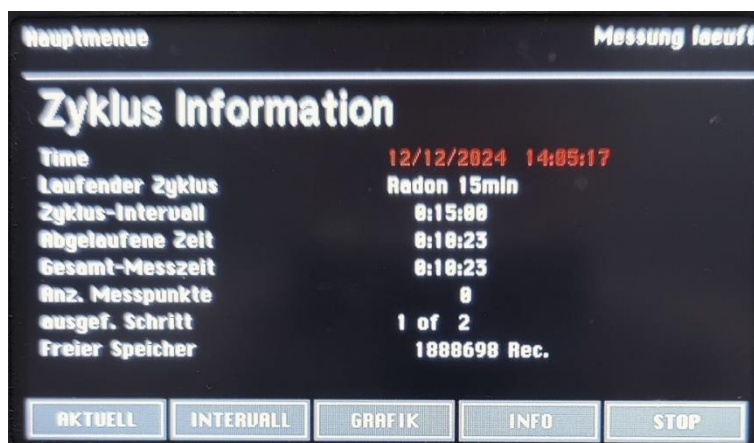


fig 4: Main menu during measurement

In "Standby" mode, the device name, the name of the current device configuration (including the date of the last change), and the selected measurement cycle are displayed. The measurement is started by touching the "START" button. While a measurement is running, the current cycle settings and system status are displayed:

- Time
- Name of the currently running measurement cycle
- Current measurement time of the current interval
- Total measurement time since the start of the measurement
- Number of the completed step and number of steps within the cycle
- Size of the free data memory (number of data records still available for storage)

From the main menu, you can also access the submenus for displaying the module and component configuration, the data stored on the memory card, and, if a measurement is running, the current measured values of the sensors.

To end a measurement in progress, touch the "STOP" button.

2. 6. 2. Display of module information and module settings

The display pages, accessible from the main menu via the "INFO" button, provide an overview of the module version and the current settings of various device parameters. The display pages can be switched using the "SHIFT" key.

Page 1 Module Information

- Software Version
- Serial Number
- Manufacturing Date
- Date of Last Firmware Update

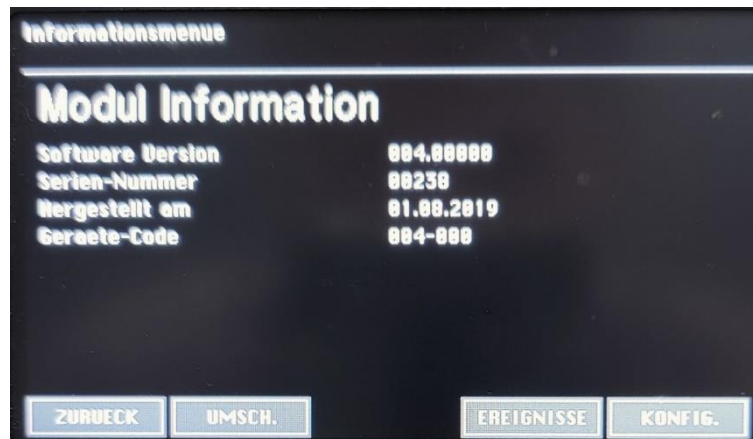


fig 5: Module information

Page 2 Module Settings

- Time of automatic start, if this function has been enabled. Otherwise, the text "disabled" appears instead of the time.
- Protocol set for the COM2 communication interface
- Information about the Wi-Fi connection stored in the device (SSID and server/port)
- Current loop output settings (data source, output signal range, and assigned value range). (The name of the data source corresponds to the unique component name. The value range refers to the physical unit of the selected measured value.)

Page 3: Additional module settings

- Timer operating mode (timer or periodic timer synchronized with the measurement cycle)
- Time points for switching the timer on and off, either as real time (timer mode) or as on, off, and delay intervals (periodic timer mode)

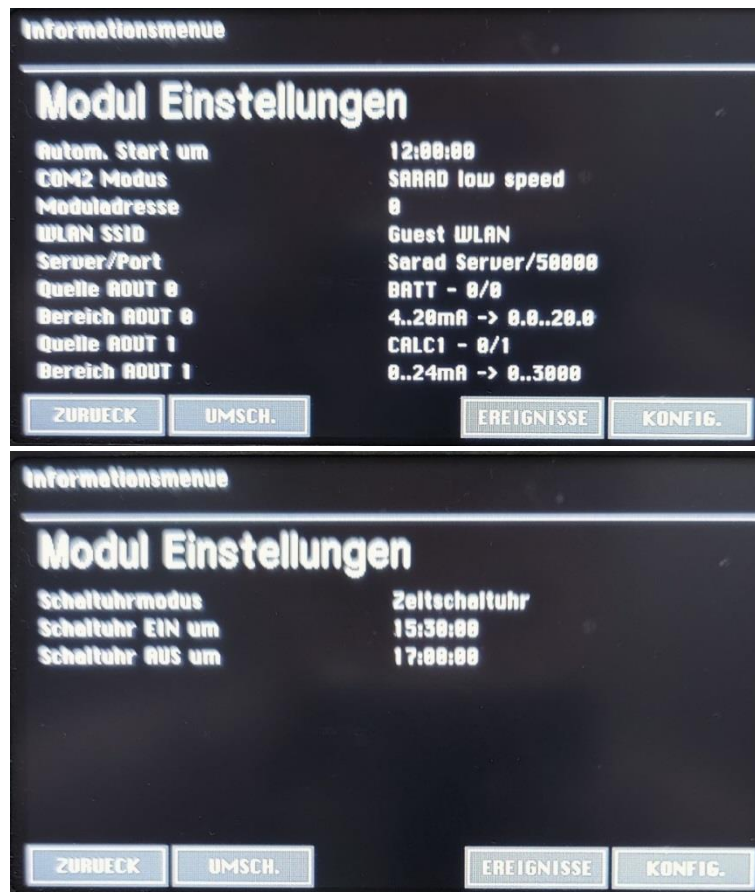


fig 6: Module settings

The "BACK" button returns to the main page. The "CONFIG." button allows you to switch to the display pages for the configured component parameters.

2. 6. 3. Display of component configuration

The current configuration parameter settings for each component can be viewed for review. To do so, click the "CONFIG." button in the information menu. Parameter changes cannot be made. The "NEXT" and "LAST" buttons can be used to select individual components.

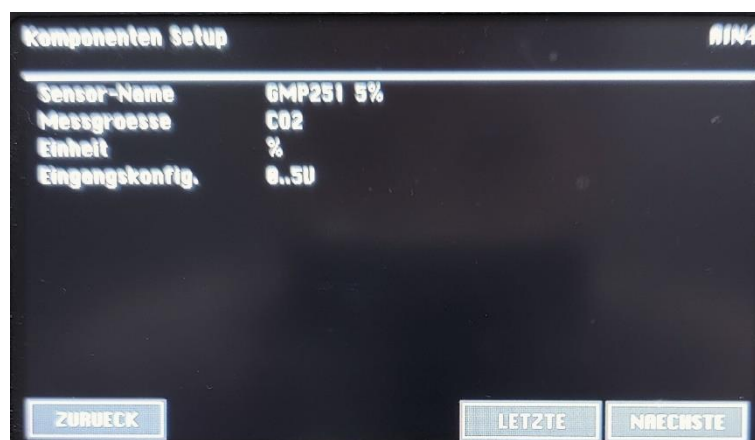


fig 7: Configuration of components

If one page isn't sufficient to display all parameters, you can access additional pages using the "SHIFT" key. You can return to the main page using the "BACK" key. The unique component name is displayed in the upper right corner.

2. 6. 4. Selection of measurement cycle

Touching the cycle name displayed in the main menu opens a list for selecting one of the predefined measurement cycles. A maximum of 15 different measurement cycles can be stored in the device. If the number of stored cycles does not fit on one display page, the "MORE" button appears, which can be used to scroll through the list. The desired measurement cycle is selected by touching the list entry. In this case, the device automatically returns to the main page. If you do not want to select a new cycle, press the "BACK" button.

2. 6. 5. Display of actual measured values

This display page is only accessible when a measurement is in progress. You access this page by touching the "CURRENT" button. The display is updated every second so that the current sample value of a component is always shown. This function corresponds to that of a direct reading measuring device. Only the data of those components that are actually included in the measurement cycle and are currently active are displayed. Switching between the available components is done using the "NEXT" and "LAST" buttons. The alias name of the component appears in the display header.

If a component delivers more than one result, the "SWITCH" button for switching the measured values is activated. Return to the main page is done using the "BACK" button.

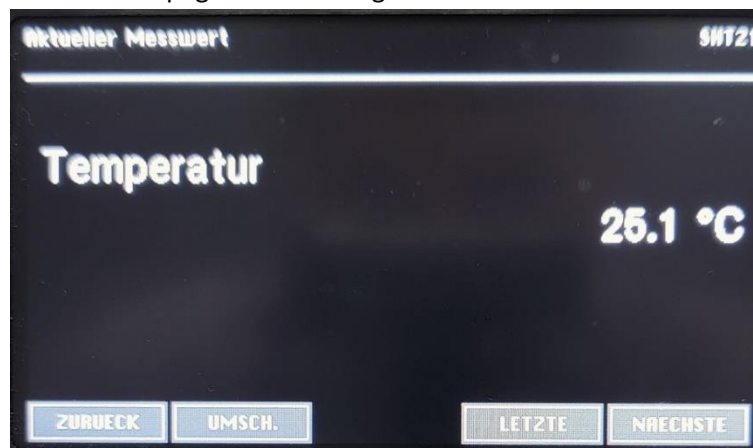


fig 8: Display of actual measured values

2. 6. 6. Display of the stored measurement values

If available, all measurement data stored on the memory card can be displayed. This function is accessible via the "INTERVAL" button during or stopped measurement. Switching between the individual components whose data is contained in the data set and selecting the desired measurement value is carried out in the same way as displaying the current values. For components that calculate multiple measured values, an additional overview page has been implemented for viewing all measurement results simultaneously.

A bar with navigation buttons appears for selecting data points within the measurement series. The middle button can be used to retrieve the most recent data set chronologically. The other buttons scroll forward or backward by one or ten data sets, respectively.

The header of the display shows the alias name of the component and the time at which the data set was saved. If the geographical position could be determined using the integrated GPS receiver, the coordinates appear in the footer. Return to the main page is achieved by pressing the "BACK" button.

In addition to the highlighted mean value of the measurement for the current measurement interval, the minimum and maximum individual values within the interval are displayed below. For radiological measurements, these two values indicate the 1-sigma confidence interval determined from the counting statistics.

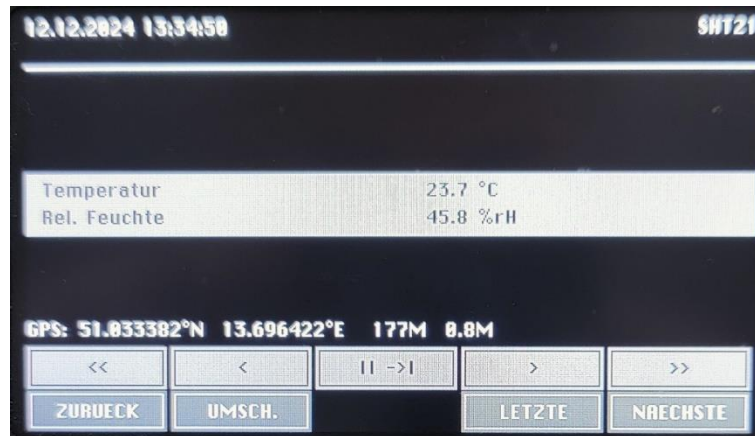


fig 9: First display page for interval measurement data for components with multiple measured values

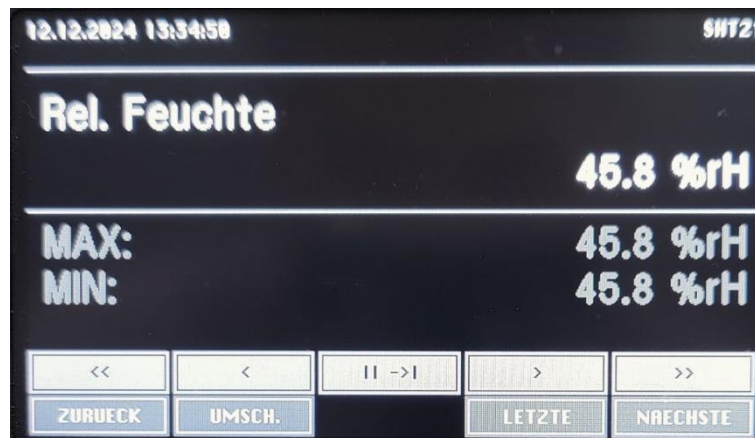


fig 10: Display of interval measurement data

2. 6. 7. Graphical display of the measurement data as a time series

All measured values available on the device can be displayed as a time series in a diagram. To do this, touch the "GRAPH" button in the main menu. The display is limited to the last 50 values of the current or most recently executed measurement cycle. The time axis is scaled accordingly until the limit of 50 measuring points is reached; after that, the oldest data is moved out of view with each new measured value during the measurement. Two measured variables can be displayed simultaneously. The Y-axis is always scaled automatically. Below the diagram view there are four navigation buttons with which the red cursor line can be moved by one or ten measured values. The timestamps and measured values associated with the cursor position appear above the cursor line. The desired measured variable is selected using the Select Y button. A table with the alias names of all available components appears. Now the desired component to be assigned to the left Y-axis can be selected. Since some components can generate multiple measured values, a list appears for selecting the desired value. The procedure for selecting the measurement value for the right Y-axis is then repeated. The "BACK" button returns to the main menu.

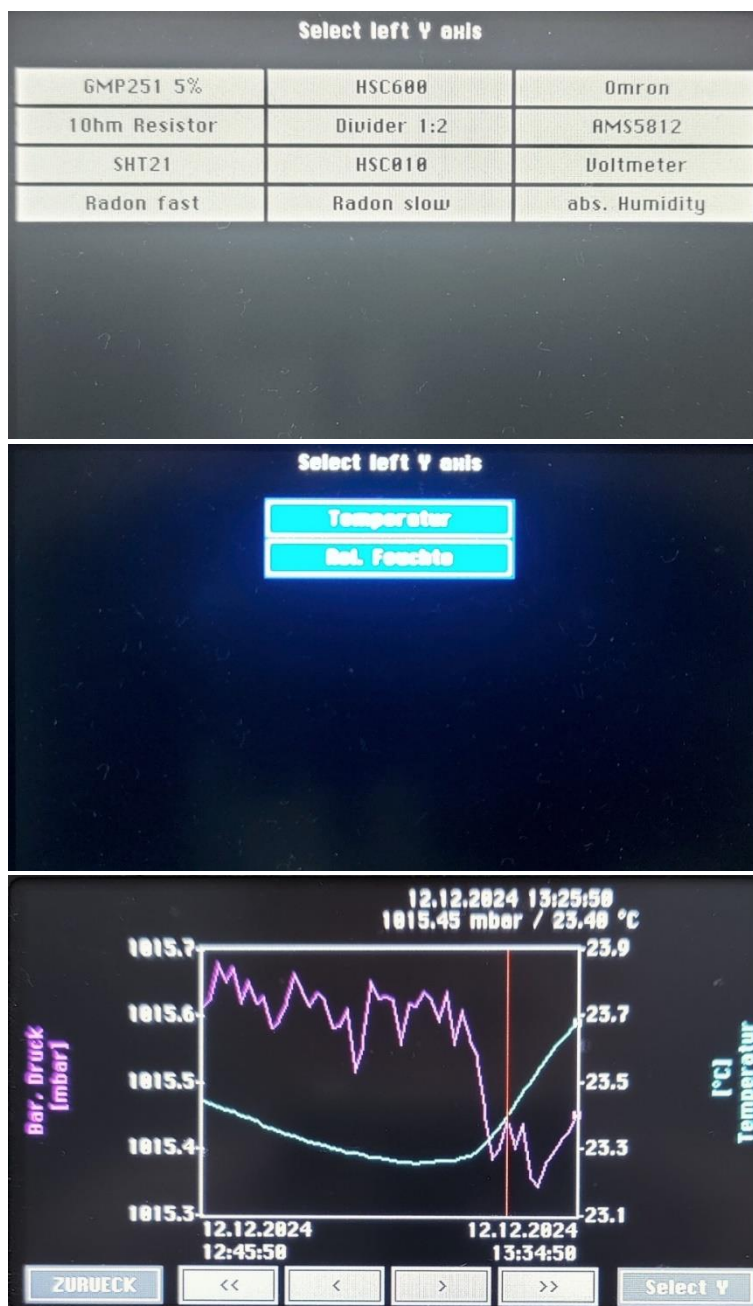


fig 11: Selection and display of series of measurements

2. 6. 8. Display of basic data

Some components support the display of the acquired base data used to calculate the displayed measured values. For such components, an additional button labeled "BASE DATA" appears on the interval data display page, which takes you to the corresponding display page.

2. 6. 8. 1. Display of the acquired spectrum

A spectrum can be displayed for all measured values that were calculated based on an acquired energy spectrum. The spectrum is shown in the form of a diagram. A control panel appears to the right of the diagram. The light grey buttons are used for cursor navigation, while the dark grey buttons are used to control the display. The upper button switches between cursor and ROI navigation. The navigation buttons can then be used to either move the cursor or switch between the energy regions (ROI) required for calculating the measured values. The "FIT Y" button scales the diagram to the maximum value of the spectrum. The "/10" and "x10" buttons can be used to increase or decrease the scaling of the Y-axis by a factor of 10. The lower button is used to switch the spectrum view between linear and logarithmic scaling.

When cursor navigation is selected, the counting channel, the associated energy, and the number of counting pulses contained in the counting channel appear above the white cursor line. When ROI navigation is selected, the energy range of the ROI is highlighted in colour. The energy range of the ROI and the counting pulses contained therein are displayed above it.

Depending on the number of counting channels in the energy spectrum, a correspondingly segmented bar appears below the diagram, allowing the spectrum to be scrolled left or right across the diagram area. The yellow bar below the scroll bar indicates the currently displayed spectrum range.

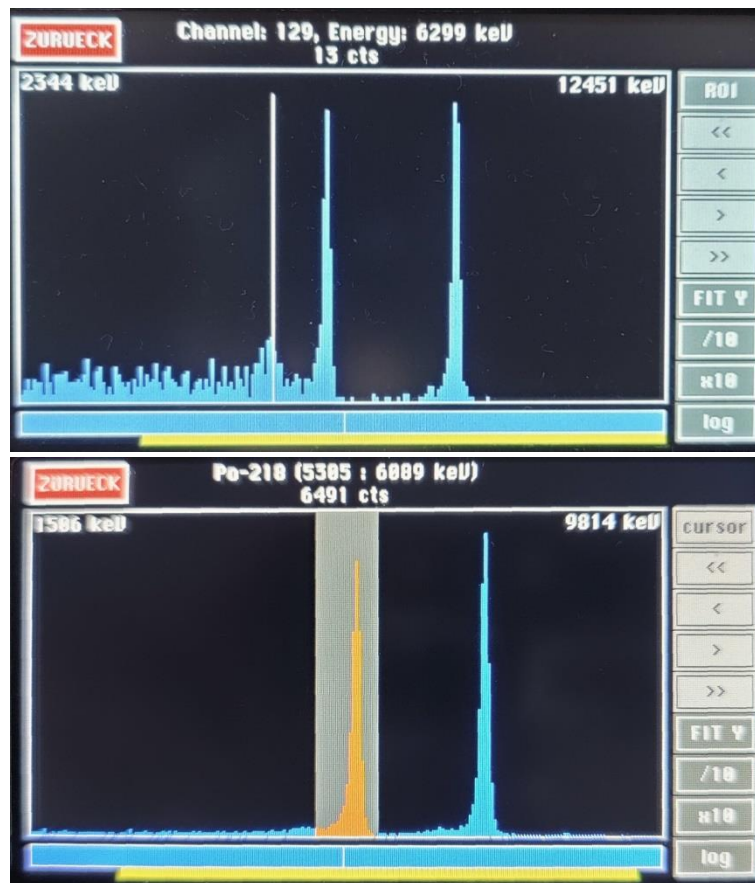


fig 12: Display of spectra (Cursor- and ROI-navigation)

2. 6. 9. Alarm-display

As soon as a new alarm occurs on the device, it automatically switches to the alarm display page. If the display was deactivated, it will be activated. The display contains a list of all existing alarms in the form of a text line. The current status of an alarm is indicated by the text colour, which is assigned as follows:

Red: New alarms, only when the alarm menu is first accessed

Yellow: Alarm situation still exists, alarm confirmation has not yet been received

Green: Alarm situation still exists, alarm has already been confirmed

White: Alarm situation no longer exists, alarm confirmation has not yet been received

The alarm is confirmed using the "CONFIRM" button in the bottom right corner of the display. The BACK button returns to the main menu. As long as alarm situations exist or there are unconfirmed alarms, a red button labelled "ALARM" appears at the top centre of the main menu. This button can be used to access the alarm display page at any time.

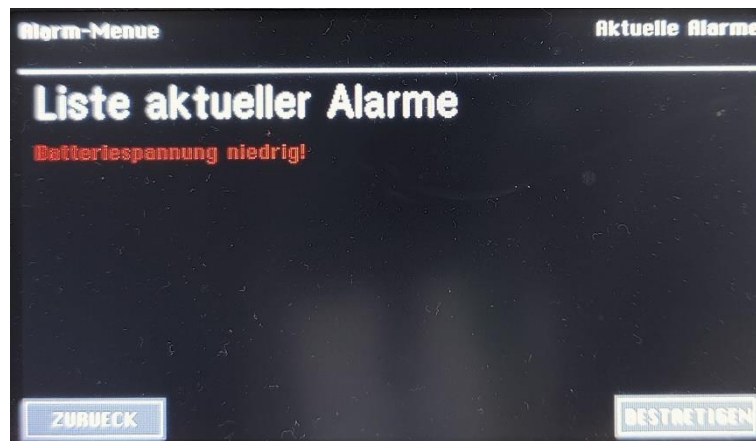


fig 13: Display of spectra (Cursor-navigation)

2. 6. 10. Display of event memory

The entries in the event log can be displayed from the main menu using the "EVENTS" button. The output is in reverse chronological order, i.e. the most recent event is at the top of the list. The "MORE" button scrolls to the end of the event list. The events are output as text messages. For some event types, the text contains additional information regarding the origin of the event, e.g. whether the event was triggered via the touch screen or via one of the communication interfaces. When selecting a cycle, the index of the selected cycle is specified. If alarms have occurred, a bit mask is displayed. The index of a component corresponds to its position within the bit mask. A set bit (a "1" is displayed) signals the origin of the alarm(s) that have occurred. The "BACK" button takes you back to the main menu.



fig 14: Display of events

2. 7. Setup (timer, synchronous start, display switch off)

2. 7. 1. Timer

Using the integrated timer, the 12VDC system voltage can be switched to an external load (e.g., relay, solenoid valve, modem, etc.) for a specific period of time. The maximum current must not exceed 400mA.

The switched voltage is available at the "AUX2" jack. The timer can operate in two modes ("Clock Switch Mode"):

1. Timer

In this mode, two times of day are specified for switching on and off. The switching process then occurs daily at these times. The device's internal real-time clock serves as the time base.

2. Periodical timer

Here, a period for the on and off states, as well as an additional switch-on delay, can be defined. The timer function is synchronized with the start of a measurement. After the start, the device waits for the switch-on delay period (which can also be set to 0). The voltage is then switched on for the switch-on period and, after this period has elapsed, switched off for the switch-off period. This process is repeated periodically until the end of the measurement. If the timer is not to be used, it can be deactivated by selecting the operating modes.

2. 7. 2. Synchronous start at a set time of day

If multiple measuring devices at different locations need to be synchronized, we recommend using the synchronous start function. A time of day can be set at which the currently selected measurement cycle will automatically start. The device's internal real-time clock serves as the time reference. The clocks of all devices to be synchronized should be set to the same time beforehand.

2. 7. 3. Display shutdown interval

To reduce power consumption, the display is deactivated after a configurable period of time (starting from the last touchscreen operation). The time period can be set from 1 to 255 seconds.

2. 8. The integrated GPS receiver

The device is equipped with a GPS receiver. The coordinates (longitude, latitude), altitude, and the deviation underlying the positioning are saved for each data set. This information is shown on the device display (interval data menu).

If the device is moved within a measurement interval, the time-weighted geographic center is saved. The current position is determined every 5 seconds, and the average values for longitude, latitude, and altitude are calculated for the entire measurement interval.

The specified deviation is an indicator of the navigation accuracy (satellite signal) underlying the positioning. The actual deviation may be greater.

Coordinates are displayed on the device in decimal degrees (max. 6 decimal places), each with the compass direction indicated.

If the reception quality is too poor, the message "No signal" appears on the display instead of the coordinates. After starting a measurement, the module needs a few minutes to acquire all satellites available for navigation.

3. Sensors and actuators in the EQF 3300

The following describes the sensors available in the device, their assignment to the DACM32 components, and the measured values generated from the sensor signals. The configuration of the respective components is not explicitly discussed, as this was defined by the manufacturer for the device. The text provides the unique component names and, in parentheses, the alias names of the components. Both names are used as needed on the various display pages.

3. 1. Radon measurement, temperature and relative humidity

The device has an internal radon measurement chamber as part of a closed air circuit between the two hose nipples "IN" and "OUT." The measuring air is pumped through the air circuit by a regulated pump with a constant flow rate.

3. 1. 1. Measuring principle

The radon activity concentration is determined based on the short-lived radon decay products formed in the device's measuring chamber. Decay products already present in the measuring air are retained by a filter system. Immediately after the decay of the radon (alpha emitter), the remaining Po-218 atom exists as a positive ion, as the emitted alpha particle tears electrons from the atomic shell. These ions are deposited on the surface of the semiconductor detector by an electrostatic field applied between the chamber wall and the detector. The number of Po-218 ions collected per unit time is proportional to the radon concentration in the measuring chamber.

Po-218, also an alpha emitter, decays with a half-life of 3.097 minutes on the surface of the detector, of which 50% of the decays (half-space) are recorded. Activity equilibrium between radon and Po-218 is reached after approximately 5 half-lives, or about 15 minutes. This determines the fastest possible response time of the device to a sudden change in radon concentration.

According to the decay sequence, the radioactive decay process continues with the two beta emitters Pb-214 and Bi-214, followed by the alpha decay of the resulting Po-214. Consequently, each Po-218 decay is detected again by the decay of Po-214 on the detector. However, this decay is delayed by the half-lives of the intervening nuclides, so that activity equilibrium between Po-218 and Po-214 is only reached after approximately two hours.

The emission energies of Po-218 and Po-214 are different, so both nuclides can be separated using alpha spectroscopy.

Spectroscopic monitors offer a choice between two methods for calculating radon concentration. In the so-called "slow mode," both Po-218 and Po-214 are included in the calculation, while in "fast mode," only the "fast" Po-218 is used.

The advantage of "fast mode" is the rapid response time to occurring concentration changes, while in "slow mode," the sensitivity (detected decays per time and radon concentration) is doubled. This increased sensitivity reduces the statistical error of the measurement, which is directly determined by the number of decays recorded within the measurement.

In the case of thoron (Rn-220), the measurement is carried out exclusively using the direct progeny Po-216. The deposition process is identical to Po-218. Since the half-life of Po-216 is less than one second, the equilibrium between thoron and Po-216 activity concentration is virtually instantaneous, and thus the measured value is available immediately.

The half-life of the Po-216 progeny Pb-212, at more than ten hours, is too long for a reasonably timely measurement, so the resulting alpha emitters Po-212 and Bi-212 are detected but not used for concentration determination. The thoron progeny products are also separated using alpha spectroscopy.

Water molecules in the measurement chamber can cause some of the Po-218 ions to recombine before reaching the detector. This results in a sensitivity dependent on the humidity, which requires appropriate compensation. For this reason, a temperature/humidity sensor is located in the device's internal air circuit to determine the humidity in the measurement chamber.

3. 1. 2. DACM32-components for the radon measurement

The amplified signal from the semiconductor detector is connected to the input of the spectrometer component SPEC1 (radon). This component separately records the count rates of the individual radon decay products Po-218 (for "fast mode"), Po-218 + Po-214 (for "slow mode"), and Po-216 (for thoron). Humidity measurement is performed by component I2C1 (SHT21), which integrates a digital humidity/temperature sensor. The radon concentration is calculated from the count rate and the measured humidity using three calculator components: CALC1 (radon (fast)), CALC2 (radon (slow)), and CALC3 (thoron).

3. 1. 3. Display of measuring values for radon, temperature and humidity

To calculate a radon measurement value, an alpha spectrum is required, which is acquired over the period of the measurement interval and is only available at its end. The calculated radon measurement values (CALC1/2/3) are therefore only displayed on the interval data display page. To make the acquisition visible during an interval, the total counting pulses of the spectrometer component SPEC1 are shown on the current data display page. Temperature and humidity values are displayed both as current measured values and as average values. Note: Since temperature and humidity are measured in the air circuit, the measurement results are only of limited use for characterizing the ambient conditions. This is particularly the case if the measuring air is drawn in from another location or if the device is heated (e.g., by sunlight or during battery charging).

3. 2. Radon/Thoron progeny measurement

For reproducible measurements of radon decay products and other radioactive aerosols, a constant flow rate ensures both consistent sensitivity and consistent airflow conditions. The latter is necessary to avoid variable particle size-dependent collection losses. The air flow is generated by an internal pump.

3. 2. 1. Functional principle

The radon decay products contained in the sample air are separated on a filter. The detector above registers the activity collected on the filter. The activities of Po-218, Po-214, and Po-212 are spectroscopically separated, and the equilibrium equivalent concentration (EEC) for radon (Po-218 and Po-214) and thoron (Po-212), as well as the equilibrium factor F, are calculated based on their count rates. To achieve practically usable response times for changes in the thoron decay product concentration, the calculation is performed by differentiating the time course of the detected Po-212 activities on the filter. Since in this case the difference between the count pulses from two consecutive measurement intervals must be calculated, the calculated value has a significantly larger statistical fluctuation range. Therefore, a correspondingly large measurement interval should always be selected. In practice, intervals of one to three hours have proven effective. These are sufficiently large to record daily cycles, for example, and are also within the response time range of the Rn-222 decay product measurement.

Note: The sensitivity of the device, i.e., the amount of decay products collected on the filter, is linearly dependent on the air flow through the filter. The device constants were determined during calibration

for the nominal flow rate specified in the data sheet. Any customer-side change to the nominal flow rate therefore requires a change to the device constants during recalibration.

3. 2. 2. DACM32-components for radon progeny

The output signal of the progeny sensor head is connected to the SPEC2 spectrometer module, which provides a spectrum for each measurement interval to determine the count rates and calculate the progeny activity concentrations. The equilibrium factor F is defined as the ratio between the radon progeny concentration and the radon concentration. The calculation is performed using the CALC3 calculator component.

3. 2. 3. Display of radon progeny products

The progeny concentrations for radon and thoron are displayed on a separate page (SPEC2), each as EEC (equilibrium equivalent concentration) and PAEC (potential alpha energy concentration). Using the toggle key, the various measured values and the corresponding confidence interval (1-sigma) can be displayed. A separate page is available for the equilibrium factor (CALC4).

3. 3. Flow measurement, flow control and pump current

For reproducible measurements of radon decay products and other radioactive aerosols, a constant flow rate ensures both consistent sensitivity and consistent airflow conditions. The latter is necessary to avoid variable particle size-dependent collection losses. The air flow is generated by an internal pump.

3. 3. 1. Functional principle

The flow rate is measured using a calorimetric mass flow sensor. This also serves as the actual value transmitter for flow control. A mass flow sensor always measures the air volume that would occupy the displayed volume under standard conditions. For example, if the ambient pressure is 10% lower, the flow rate must also be increased by 10% to achieve the same air flow rate. The measuring air flows through the flow sensor as part of the internal air circuit. The control loop gradually increases or decreases the pump flow if the sensor's measured value deviates upwards or downwards from the nominal flow (setpoint). If the filter is too heavily contaminated, the pump reaches its maximum capacity, so that further contamination will prevent the nominal flow rate from being achieved. Therefore, the device's alarm system generates a warning signal at 80% of the pump capacity.

Every pump is a mechanical component subject to wear. At the end of its service life or in the event of a defect, the pump's operating current can increase significantly, even leading to a short circuit. To protect the electronics, the device monitors the pump current and the alarm system stops the measurement if a limit value is exceeded.

3. 3. 2. DACM32-components for internal air circuit

The flow sensor output is connected to analog input AIN6, and the pump current and pump voltage signals are connected to analog inputs AIN6 and AIN7. The pump power is controlled by the controller component REG1. The controller component generates a control voltage that can be used to vary the pump power.

3. 3. 3. Display of the measured values of the air circuit

The current flow rate measurement (AIN6) and the pump current (AIN7) are displayed in the corresponding physical unit. The pump voltage (AIN8) serves as an indicator of the required pump power and thus the condition of the filter. The maximum possible pump voltage determines the maximum pump power and thus the control limit for the flow. The control limit is equated with a filter

occupancy of 100%. A new filter would theoretically correspond to a filter occupancy of 0%. However, the lower value is factory-set to 15%, as the required pump power can vary within certain limits depending on the ambient conditions and filter. Instead of the pump voltage, the device displays the filter occupancy in percent. Each measured value of the air circuit has its own display page.

3. 4. Barometric pressure, differential pressure (option)

The device is equipped with a barometric pressure sensor as standard, and an optional differential pressure sensor for small differential pressures. In the standard device, the pressure sensor terminal is connected to the device's centre tube nipple labelled "p." If a differential pressure sensor is present, the vacuum sensor terminal is connected to the hose nipple. The unconnected terminals are open, i.e., they are subjected to ambient pressure. Note: The pressures applied to the "p" hose nipple must not exceed the maximum permissible pressure values specified in the data sheet. The I2C2 component is used for the barometric pressure sensor; for the optional differential pressure sensor, the analog input AIN5 or the I2C3 component is used, depending on the configuration. The pressure values are each displayed on a separate display page.


3. 5. Warning and alarm lights

The basic unit has a signal LED labelled "!" directly above the "WAKE" button. This LED illuminates both in the event of warnings and alarms. The signal LED is connected to the DOUT8 switching output. Two additional signal lights can be connected to the "AUX2" socket. A signal tower (yellow/red combination) is included upon request, or two separate signal lights (yellow and red) can be mounted on the lid of the measuring case. The yellow light indicates warnings regarding the operating status of the device (DOUT1), while the red light (DOUT2) is assigned to radiometric alarms.

3. 6. The connectors „AUX1“ and „AUX2“


The two accessory connectors allow the connection of external sensors and actuators, as well as accessories for special measurement tasks. Caution: Only components supplied by SARAD may be connected to these two sockets. Improper use may damage the device's electronics.

The "AUX1" socket is primarily intended for connecting radiation sensors, while the "AUX2" socket provides external connections for various DACM32 components. The following tables show the socket assignments and signal usage in the EQF 3300.



Socket "AUX1" (Binder Series 712, 5-pin), front view of the socket

Pin	Signal	Use
1	SPEC2	Pulse input for spectrometer component, detector signal of the progeny product measuring head
2	V+	supply voltage for progeny product measuring head
3	CMP1/CNT1	Comparator/counter combination, not used in EQF 3300
4	BIAS	Bias voltage for progeny measuring head
5	GND	Reference potential



Socket „AUX2“ (Binder Series 680 – DIN 8-pin), front view of the socket

Pin	Signal	Use
1	DOUT1	Switching output for optional accessories, controlled by the alarm system. A voltage of +12VDC is applied when activated.
2	AIN1	Analog input , no use in EQF 3300
3	AGND	Reference potential for AIN1, AIN2, and CMP1, no use in EQF 3300
4	DOUT2	Switching output for optional accessories, controlled by the alarm system. A voltage of +12VDC is applied when activated.
5	AIN2	Analog input, no use in EQF 3300
6	Clock-Switch	Switching output of the timer. A voltage of +12VDC is applied when activated, no use in EQF 3300
7	PGND	Reference potential for +12VDC, Ground wire for red and yellow signal lights
8	DIN1	Digital status input for optional accessories

4. EQF 3300 device configuration

4.1. Predefined measuring cycles

The following measuring cycles are stored in the delivered device:

Name of cycle	Description
Rn+FP 15min	Continuous radon/thoron and radon/thoron progeny measurement with 15-minute measurement intervals
Rn+FP 30min	Continuous radon/thoron and radon/thoron progeny measurement with 30-minute measurement intervals
Rn+FP 1h	Continuous radon/thoron measurement and radon/thoron progeny measurement with 1-hour measurement intervals
Rn+FP 2h	Continuous radon/thoron and radon/thoron progeny measurement with 2-hour measurement intervals
Signal-Test	Test the "!" signal LED and, if present, the external signal lights (flashing)

4. 2. Predefined warnings and alarms

The DACM32 platform offers a highly flexible alarm system that allows any user-specific alarms and warnings to be generated. The following alarms are configured by default:

Measuring value (Alarm-source)	Hint	Signal	Alarm message
Pump controller (AIN8)	Pump capacity >80%	LED front plate, ext. Yellow lamp	"Air inlet blocked or water inlet protection!"
Battery voltage (BATT)	Battery voltage less than 11.6V	LED front plate, ext. Yellow lamp	"Battery discharged, please charge!"
Pump current (AIN7)	Pump current >300mA	Measurement will be stopped immediately	Alarm can be read in the event log
Optional: Differential pressure (AIN5 or I2C4)	Differential pressure too low (e.g., if no filter was inserted or hose is not connected)	LED front plate, ext. Yellow lamp	"No pressure drop, check filter!"
Radon concentration (SPEC1)	Check at the end of the measuring cycle	LED front plate, ext. red lamp	„Radon limit exceeded“
Radon progeny product concentration EEC (SPEC2)	Check at the end of the measuring cycle	LED front plate, ext. red lamp	„EEC limit exceeded“
Humidity sensor (I2C2)	Humidity in the internal air circuit >96%	LED front plate, ext. red lamp	"Risk of condensation!"

Hint: The alarm check is only possible if the component that provides the measured value is activated in the measurement cycle. When defining custom measurement cycles, ensure that all components listed in the table are activated.

The battery voltage is monitored independently of the alarm system. At a voltage of 11.2V, the measurement is automatically stopped without additional signalling. A corresponding entry is made in the event log.

The alarm signalling with yellow and red external lights is only activated if the device is supplied with a measuring case or a light column (accessory).

5. Important hints on operating the device

5. 1. Vibrations and strong electromagnetic fields

Continuous strong mechanical shocks and vibrations can affect the detector signal due to the piezoelectric effect and must be avoided. The device should not be operated in close proximity to strong and high-frequency electromagnetic fields (e.g., placing the device on high-voltage switchgear or placing mobile phones on the device).

5. 2. Aggressive Gases

Due to the operating principle, all sensors, semiconductor detectors, and mechanical components come into contact with the measuring air. Aggressive gases can damage or destroy the sensitive surfaces of the sensors/detectors or contact systems. This can lead to measurement errors or malfunction. Avoid using the device in the presence of aggressive gases.

5. 3. Environmental conditions

The ambient conditions specified in the data sheet must be observed. Operating outside the specified limits may result in incorrect measured values or limit the functionality of the device. If the device must be used under such conditions, please consult the manufacturer.

5. 4. Control of the alpha spectra

Recording and displaying alpha spectra is the most powerful tool for quality assurance of radon and progeny measurements. Both the radon measurement chamber and the progeny sensor head provide characteristic energy spectra that the user can reliably evaluate after a short period of time. All radon and thoron progeny generate characteristic peaks in the spectrum, the shape and position of which indicate the proper functioning of the device. Less experienced users should save the initial measurement results after delivery of the device so that "reference spectra" are available for later comparison. A quick look at the acquired alpha spectra should always be part of good measurement practice.

5. 5. Avoiding condensation

The formation of condensation in the device must be avoided. Condensation can occur if the device temperature is below the temperature of the measuring air and the dew point is exceeded upon cooling. Typical scenarios are soil air measurements in winter or immediate measurements in humid, warm rooms after transport at low temperatures. In such cases, the device must be sufficiently warmed before use. Damage to the device is not expected, but it may impair the measurement. If, for example, constant temperature changes are expected in a stationary installation under humid ambient conditions, a cooling and condensation device must be installed upstream or the device must be placed in a heated measuring cabinet. Depending on the device type, rotary vane pumps are used to generate the airflow. The surfaces of the compressors can corrode if surface moisture is present, which can lead to reduced pumping performance or even inoperability. After measurements under humid conditions, a fifteen-minute measurement should be performed in a dry environment to remove any moisture present from the internal air circuit.

5. 6. Water ingress protection

Especially when measuring soil gas or water samples, it is important to ensure that no water can enter the internal air circuit. The pump's power is sufficient to suck water even from deeper sample boreholes. In this case, all sensors come into direct contact with water. For this reason, the water inlet protection must always be used. This is included with the "Soil Gas" and "ULTRA" versions of the device and is available as an accessory for the standard device. This consists of a container with a float switch that is inserted between the sampling device and the air inlet of the device. If water enters, the float switch switches off the pump via an additional socket on the device. Note: The container must always be used vertically, i.e. with the connections pointing upwards (for devices with a retaining clamp for the water inlet protection, the device must be operated in the appropriate position). It is recommended that a functional test be carried out before each use. To do this, start a test measurement and then turn the empty container with the connections facing downwards. The pump must stop immediately.

If water is accidentally sucked in, first disconnect the hose connecting the container to the air inlet. Then, disconnect the second hose from the container and the connecting cable from the device. The container can now be removed from the holder, unscrewed (turn the lid clockwise), and emptied. The surfaces should be dried with a cloth. Any water contained in the hoses should also be removed. When closing the container lid, ensure that the rubber seal is correctly seated. The container should be checked for leaks.

5. 7. Filter at the air inlet of the device

The internal gas circuit contains a multi-stage filter to prevent radon decay products already present in the sample air from entering the radon measurement chamber. This filter is not accessible from the outside and is normally maintenance-free. This requires that dust and other particles are removed from the sample air beforehand. If the decay product measuring head is not used, the supplied syringe filter should be connected to the device's air inlet instead. This filter should be replaced if significant contamination is visible or if the required pumping capacity is significantly increased.

5. 8. Rechargeable battery

The lifespan of the built-in battery is reduced if it is deeply discharged or stored in a discharged state for extended periods. Even a fully charged battery will reduce its lifespan. For this reason, the battery should be subjected to a charge and discharge cycle every three months. This also applies if the device is not used for an extended period of time (the battery is subject to slight self-discharge, i.e., it loses capacity even when no power is drawn). Before the device is not used for an extended period of time, the battery should be charged to approximately 13V, the device turned off, and the fuse removed. Note: Deep discharge of the battery usually leads to a defect. This is detected by the charger, so the charging process will not begin.

5. 9. Hints for the sampling head for progeny products

5. 9. 1. Connection and placing

The progeny sampling head is a separate unit that can be mounted on a rod and placed in the room. A rod thread is provided on the underside of the measuring head for this purpose. The airflow through the filter is generated by the base unit, so the air connection of the measuring head must be connected to the air inlet of the base unit with a special tube. Furthermore, the electrical connection to the device must be established by plugging the connecting cable into the "AUX1" socket on the front panel. The connectors must be locked with the screw sleeve, and the tube connection must be checked for leaks. Depending on their size distribution, aerosols can adhere to surfaces solely through thermal movement, leading to a depletion of aerosols and radon progeny in the surrounding area. Therefore, the progeny measuring head should be placed as far away from surfaces as possible.

5. 9. 2. Change of the filter

The filter must be changed at the latest when a corresponding warning appears on the device. Changing the filter sooner is recommended, as increasing contamination increases the pump's energy consumption and reduces the device's battery life.

To change the filter, first pull out the swivel arm and swing it away (left image). Then, the filter lock can be opened by simultaneously pressing and turning the inner ring (centre image). The filter can now be removed and replaced with a new one. A neoprene seal is applied to the back of the filter. The front side must face the detector during operation. Only filters specified by SARAD may be used. This ensures the system's tightness and the required spectroscopic resolution.

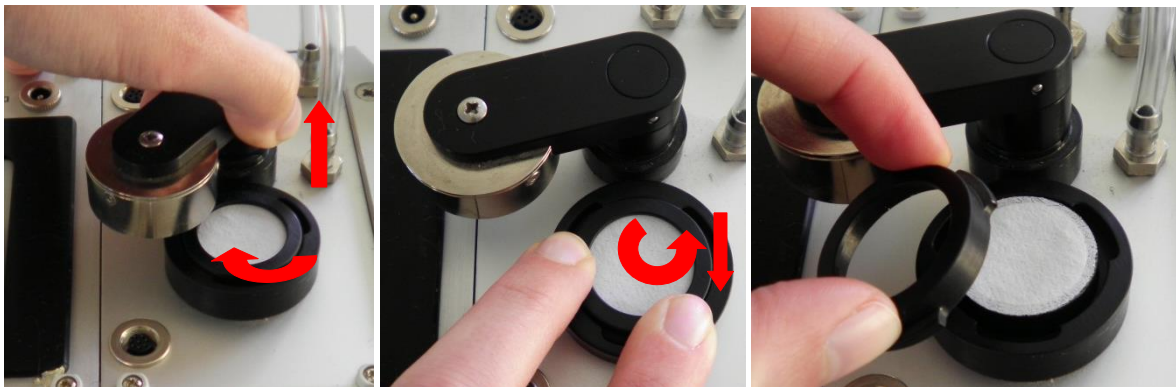


Fig. 15 Change of the filter

5. 9. 3. Detector cleaning and protection

In very dusty environments, the detector surface becomes contaminated, as a small portion of the aerosols is always deposited and accumulated on it. Cleaning must be carried out with extreme caution, as even small scratches on the detector surface can destroy the light shield and render the detector unusable. Any dust should be removed with a very soft optician's brush. Under no circumstances should the surface be wiped or liquids used for cleaning. If use in a dusty environment is necessary, the optionally available detector protection should be used. This consists of a thin film that is stretched over the radiation entrance window of the detector using a tensioning frame. A bracket positioned above the pivoting arm holds the tensioning frame in position using two screws. The film can be easily replaced by the user. To do this, the tensioning frame and the old film must be

removed before a new film is carefully placed centred over the radiation entrance window of the detector. Placing the tensioning frame in place smooths the film. The bracket can now be attached and the tensioning frame secured with the two screws.

Note: Only films specified by SARAD may be used, as the film influences the spectroscopic properties of the measuring setup.

6. Use of accessories

6.1. Accessory adapter

For some accessories (e.g. water ingress protection) it is necessary or advisable to permanently connect them to the device. For this purpose there is an accessory adapter on the left side panel of the housing. This has a central threaded M6 hole for fastening and a series of opposite holes for positioning the accessories. The attachment is made using the counterpart that matches the respective accessory, which has two tabs for the positioning holes and a central hole for fastening with an M6 screw. The positioning holes are arranged in such a way that vertical positioning is guaranteed when the device is lying down (rack), standing up (case) and when using the stand bracket (table). The user must make the appropriate adjustment depending on the position of the device.

6.2. Measuring case for harsh environmental conditions

If the device is to be used in harsh environmental conditions, the use of the optionally available measuring case is recommended. This is dust- and waterproof and features tube connections for transporting the measuring air to and from the device. The power supply socket on the case allows continuous operation of the device with the case closed (the cable extension in the case must be plugged into the "DC" socket). Depending on the model, one or two signal lights are mounted on the top of the case lid to indicate warnings and alarms. The connection cable for the signal lights is connected to the "AUX2" socket on the front of the device. When closing the case lid, care must be taken to ensure that no air tubes or cables are kinked. The measuring case for the EQF 3300 has an additional hole for the connection cable and the installation of the downstream product measuring head. The connection cable must be connected to the "AUX1" socket accordingly.

Note: The Rn/Th progeny sampling head itself is not protected against water ingress. If there is a risk of dripping water occurring at the measuring location, appropriate protective equipment must be provided.

6.3. Light column

The light column is used to signal warning and alarm conditions. The bright 360° signal lights ensure good visibility even from greater distances. The light column is connected to the device's "AUX2" socket. It is controlled via the "DOUT1" (yellow) and "DOUT2" (red) switching outputs. The light column can be freely positioned in the room using either a mounting bracket on the device's accessory adapter or a suitable cable extension.

Attachment

A) DACM32 components

A1 – Type of components of DACM32

Type	Name	Description
Analog input	AIN	Connects sensors with analog output signals (0...1V, 0...2V, 0...5V, 0...10V, 0/4...20mA).
Status input	DIN	Detects states (e.g., switch contacts), recording the on and off duration and the number of changes.
Comparator-input	CMP	Detects pulse signals that are greater than an adjustable threshold; used in conjunction with a counter input.
Counter input	CNT	Detects a total number of pulses, a pulse rate, or an average pulse rate. Will be used with sensors with a pulse output.
Spectrometer	SPEC	Spectrometer module for recording pulse height spectra.
Universal digital sensor interface	I2C	Connects sensors with a digital interface according to the I2C standard.
Controller	REG	Provides a PID control loop. All available measurement results from existing sensors serve as the setpoint, and a control voltage is output at the controller output.
Switching output	DOUT	Potential-free switching contacts (opto-MOS switch or relay changeover switch)
Frequency generator	PWM	Applies a square-wave signal with variable pulse width to the output.
Calculator	CALC	Calculates complex measurement results from the measured values of the available sensors using functional prototypes.

A2 – Overview of the used components in EQF 3300

Name	Alias-Name	Function
AIN1	AUX2-Pin2	Signal at "AUX2" jack, unused
AIN2	AUX2-Pin5	Signal at "AUX2" jack, unused
AIN5	Delta-p	Differential pressure, depending on the measuring range AIN5 or I2C3 (only with the "differential pressure sensor" option)
AIN6	Air-flow	Flow measurement and setpoint for flow control
AIN7	Pump current	Measurement of the internal pump current
AIN8	Filter assignment	Measurement of filter occupancy based on the pump voltage
CMP1	AUX1-Pin3	Unused, Signal at „AUX1“ socket, internal connection to CNT1
CNT1	AUX-CMP1	Internally connected to the output of CMP1, unused
DIN 1	AUX2-PIN8	Unused, at socket AUX2
SPEC1	Radon chamber	Connected to the detector signal of the radon measurement chamber, it generates an alpha spectrum and determines the count rates of the individual nuclides. Display: R Po-218, R Po-218/214, R Po-216
SPEC2	Rn/Th progeny	Connected to the progeny sampling head, generates alpha spectrum and calculates EEC/PAEC


I2C1	AMS5812	Measurement of barometric pressure
I2C2	SHT21	Combined temperature and humidity measurement in the internal air circuit
I2C3	Delta p	Optional Differential pressure sensor for filter control
REG1	Pump controller	Controls the flow via the pump power
DOUT1	AUX2-Pin1 or Signal yellow	Signal to socket "AUX2", either unused or connection of the yellow signal light on the measuring case
DOUT2	AUX2-Pin1 or Signal red	Signal to socket "AUX2", either unused or connection of the red signal light on the measuring case
DOUT6	High voltage	Switches on the high voltage for radon measuring chamber
DOUT7	Pump voltage	Switches on the supply voltage for pump and pump control
CALC1	Radon (fast)	Calculates the radon concentration (Fast-Mode) from Po218-count rate
CALC2	Radon (slow)	Calculates the radon concentration (Slow-Mode) from the sum of the count rates of Po218 and Po214
CALC3	Thoron	Calculates the Thoron concentration from Po216-count rate
CALC4	EQF	Calculates equilibrium factor for radon and its decay products

B) Connector pin assignment



2 x 4-20mA

Pin	Signal	Description
1	AOUT1+	Current Loop 1 Output
2	GND	Common reference potential (-) for AOUT1 and AOUT2
3	AOUT2+	Current Loop 2 Output
4	GND	Common reference potential (-) for AOUT1 and AOUT2




RS485A/RS485B (RJ45 Buchse, 8-pin)

Pin	Signal	Description
4	B/B'	Transceiver terminal 1, V1 voltage (V1 > V0 for binary 1 [OFF] state)
5	A/A'	Transceiver terminal 0, V0 voltage (V0 > V1 for binary 0 [ON] state)
8	GND	Reference potential
1, 2, 3, 6, 7	N.C.	Not used



RS232 (SUB-D Buchse, 9-pin)

Pin	Signal	Description
2	TX	Device's transmit line (output)
3	RX	Device's receive line (input)
5	GND	Reference potential
1, 4, 6, 7, 8, 9	N.C.	Not used



DC (2,5mm jack socket)

Pin	Signal	Description
Inside	20VDC	Power supply and charging voltage
Housing	GND	Reference potential

C) Disposal instructions

Batteries and accumulators must not be disposed of in the trash, but must be disposed of at local collection points!

At the end of their service life, the measuring devices must be disposed of as electronic waste or returned to the manufacturer for proper disposal! If necessary, decontamination must be carried out before disposal.